


* sold separately

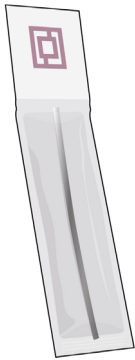

Intended Use: The VERIFY™ DualAction Ultrasonic Indicator is intended to verify the ultrasonic activity and performance of ultrasonic cleaners operating in the frequency range of 38 - 40kHz. It is intended to be used in conjunction with the LCC028 VERIFY DualAction Ultrasonic Indicator Holder as a daily check of an ultrasonic cleaner using a standard basket and no instruments.


Important: • Check Indicator expiration date • Ensure the holder is clean and dry • Ensure gloves are clean and dry before handling the indicator. • Single use only, do not reuse processed/partially processed indicators due to a risk of a false Pass result.

Disposal: This product may be disposed of as regular waste.


Note: Serious incidents that have occurred in relation to this medical device should be reported to the manufacturer and competent authority in the country where the incident occurred.

Instructions for use


d1

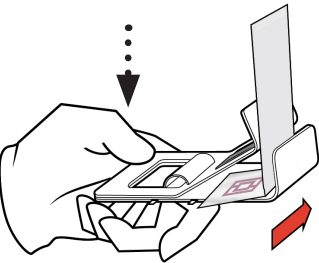

d2


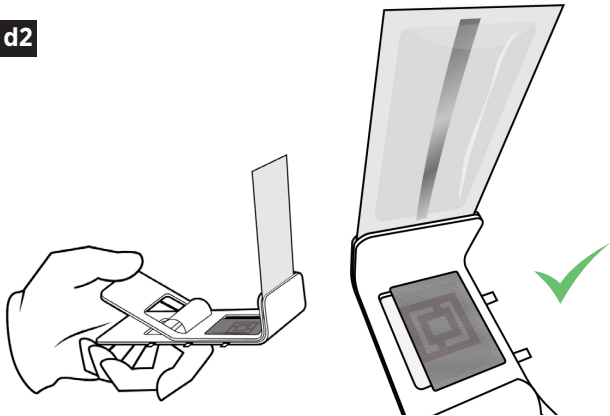


d3

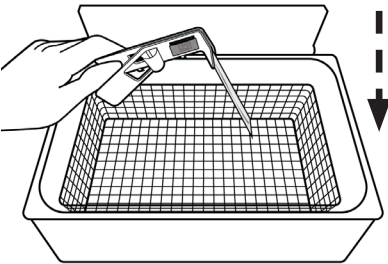


d4*

Orientation and placement example only. Location(s) shown in the table in the user reference guide (M13590GB.2024-09, Rev.A)

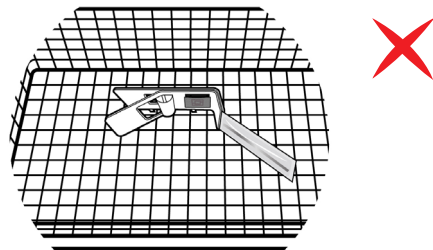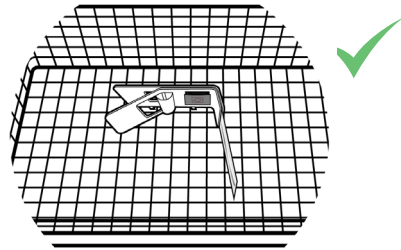


d5*


Start the dedicated program



d6



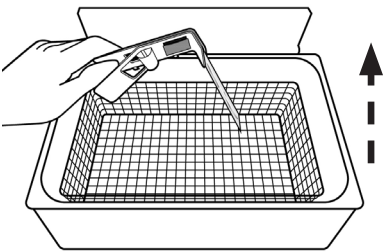


d7*

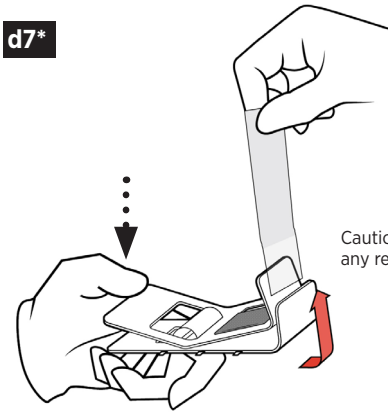

Caution, as the holder may be hot and any residual soil may stain.

d8

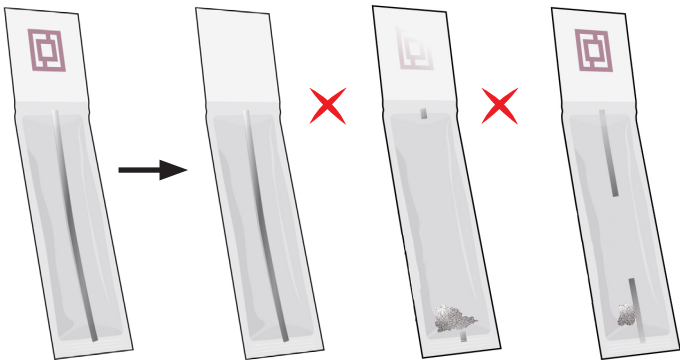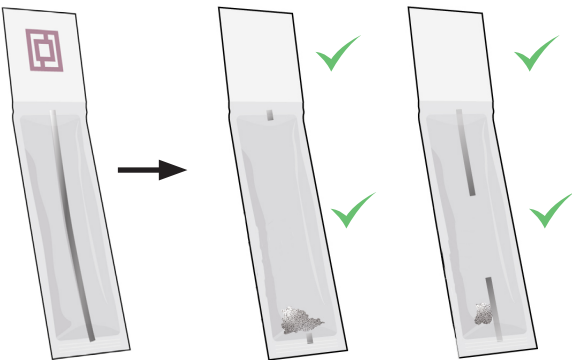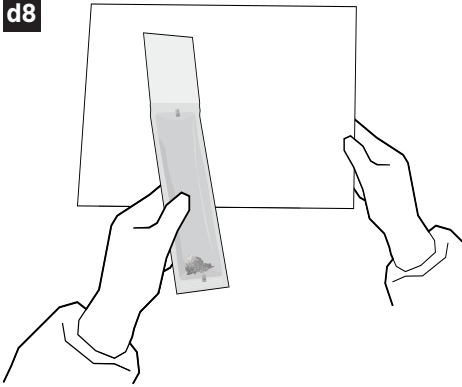

(en) In the event of a Fail, departmental procedures should be followed. (da) I tilfælde af fejl skal afdelingsprocedurer følges. (de) Im Falle eines „Fail“-Ergebnisses sind die Verfahren der jeweiligen Abteilung zu befolgen. (es) Siga los procedimientos de su departamento para informar de los fallos. (fi) Vikatapauksessa on noudatettava osastokohtaisia menettelyjä. (fr) En cas de défaillance, les procédures du département concerné doivent être suivies. (it) In caso di mancato superamento, seguire le procedure dipartimentali. (ja) 不合格の場合は、各部門の手続きに従うこと。 (ko) 불합격이 발생하는 경우, 부서 절차를 따라야 합니다. (no) Ved feil skal avdelingens prosedyrer følges. (pl) W przypadku awarii, należy postępować zgodnie z procedurami zakładowymi. (pt) Em caso de Falha, devem ser seguidos os procedimentos do serviço. (sv) I händelse av ett underkännande ska avdelningens rutiner följas. (th) ในกรณีที่เกิดเหตุขัดข้อง ควรปฏิบัติตามขั้นตอนของแผนก (tr) Bir arıza durumunda departman prosedürleri takip edilmelidir. (zh) 如果出现故障，应遵循部门程序。 (zh) 如果出现故障，請遵循部門規程。

[illegible]